



C/ Luis Fuentes Bejarano 60 Ed. Nudo Norte
(local 3) 41020 Seville - Spain

Phone: +34 954 93 32 00
pedidos@vitro.bio
www.vitro.bio

Gene rearrangements analysis for the diagnosis of **lymphoid diseases**



Gene rearrangements analysis for the diagnosis of lymphoid diseases

- Based on PCR amplification
- Monotest format of PCR mixes in color-coded 0.2 ml tubes
- All amplifications are carried out under the same PCR conditions
- Hot Start II DNA Polymerase is supplied in the kit
- Internal amplification control for checking the quality of the DNA
- Positive controls for clonal and polyclonal DNA are supplied in the kit
- Primers are marked at their 5' end with 6-FAM fluorochrome
- Optimized for paraffin embedded tissues
- Total run time 3 hours
- 100% concordance with the expected results in EuroClonality/ Biomed 2.
- External Quality Assessment

DESCRIPTION

IgH Rearrangements Molecular Analysis Kit (20 test)

TCR Gamma Rearrangements Molecular Analysis Kit (20 test)

TCR Beta Rearrangements Molecular Analysis Kit (20 test)

IgK- IgL Rearrangements Molecular Analysis Kit (20 test)

REFERENCES


MAD-003994BP-2

MAD-003994TP-2


MAD-003993TP-2

MAD-003999M-2


IgH

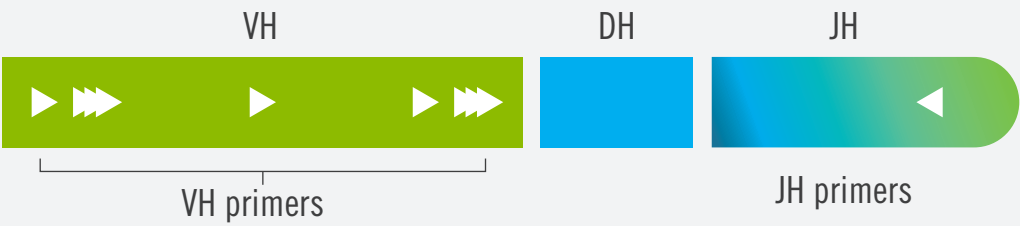

TCR γ

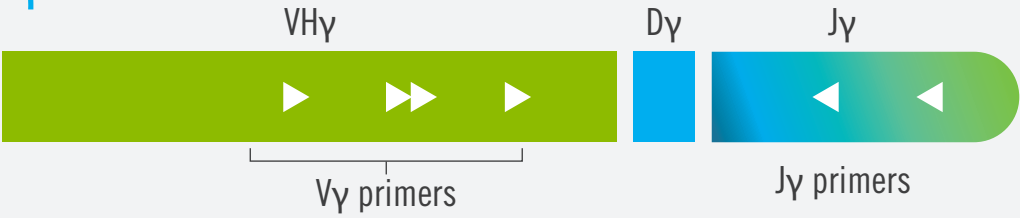

TCR β

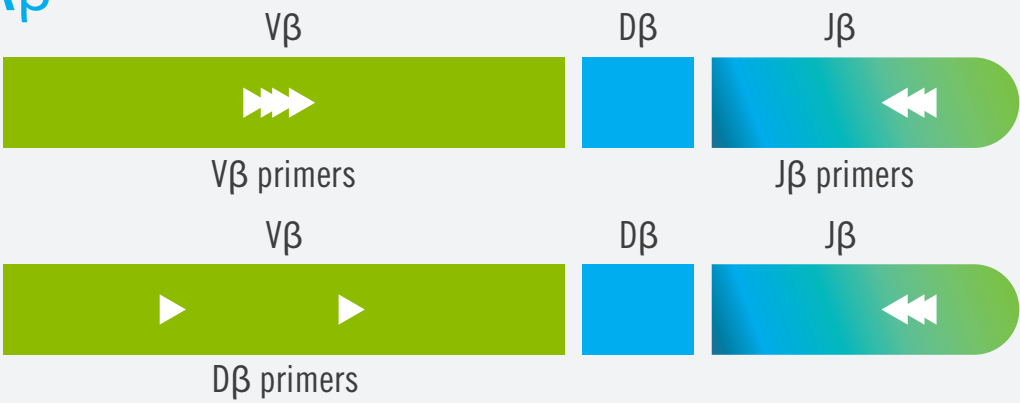

IgK-IgL

